

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-11

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA				MS	Others	
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	1,283	1,283							
3014	1,388							1,388	
3019	1,431								1,431
3025	1,330							1,330	
3027	1,496							1,496	
3028	1,440								1,440
3030	1,337							1,337	
3031	1,482								1,482
3033	1,341		1,341						
3035	1,470		1,470						
3036	0,938						0,938		
3037	1,257							1,257	
3038	1,558							1,558	
3039	1,290							1,290	
3040	1,333		1,333						
3041	1,420								1,420
3047	1,243							1,243	
3048	1,405		1,405						
3049	1,324							1,324	
13004	1,260	1,260							
15033	1,440							1,440	
20002	0,870		0,870						
30001	1,685							1,685	
30003	1,278	1,278							
30005	1,540							1,540	
30006	1,452			1,452					
40001		[3,724]							
40003-1	1,782	1,782							
40003-2	2,120							2,120	
40004	1,181							1,181	
40013	2,520					2,520			
40014	1,347							1,347	
40015	2,860				2,860				
40016	2,600				2,600				
40017	2,240					2,240			
40018	1,188		1,188						
40020	1,440								1,440
40021	1,205		1,205						
40023	2,260						2,260		
40024	1,270	1,270							
40025					[0,0064]				

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-11



Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	1,320		1,320						
40029	2,800				2,800				
40031	1,410								1,410
40036	1,185		1,185						
40037	1,260		1,260						
40041	2,450				2,450				
40043	1,638			1,638					
40047	1,205		1,205						
40049	1,165		1,165						
50001	1,295		1,295						
50002	1,417		1,417						
60005					[5,833]				
60006	0,909							0,909	
70001	1,088		1,088						
70002	1,250		1,250						
70003	1,490		1,490						

Statistical Results

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	1,503	1,375	1,262	1,545	2,678	2,380	1,599	1,403	1,437
SD	0,455	0,228	0,147	0,132	0,188	0,198	0,935	0,261	0,025
Mean - 2SD	0,594	0,919	0,967	1,282	2,301	1,984	0,000	0,882	1,387
Mean + 2SD	2,413	1,830	1,556	1,808	3,054	2,776	3,469	1,924	1,487
Amount	54	5	18	2	4	2	2	16	6

*The graphic is for information purposes only and not validated. Please read your results from the table.

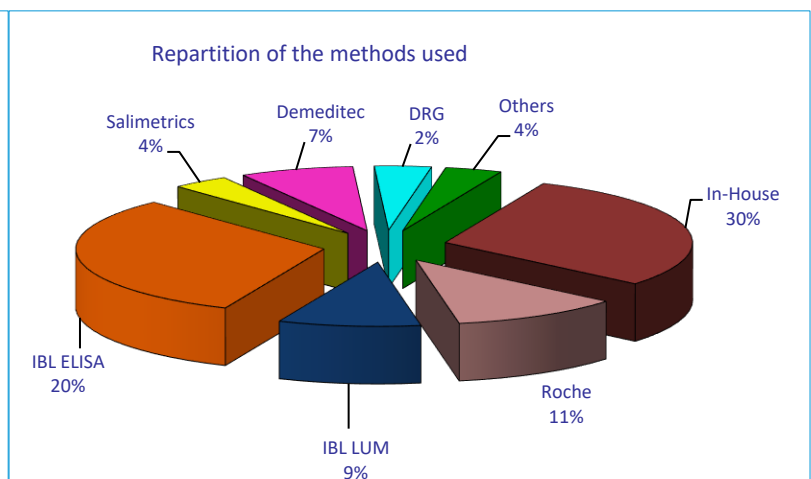

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-12

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	0,074	0,074							
3014	0,083							0,083	
3019	0,065								0,065
3025	0,061							0,061	
3027	0,071							0,071	
3028	0,079								0,079
3030	0,065							0,065	
3031	0,079								0,079
3033	0,091		0,091						
3035	0,040		0,040						
3036	0,036						0,036		
3037	0,069							0,069	
3038	0,072							0,072	
3039	0,058							0,058	
3040	0,069		0,069						
3041	0,098								0,098
3047	0,069							0,069	
3048	0,122		0,122						
3049	0,065							0,065	
13004	0,070	0,070							
15033	0,070							0,070	
20002	0,029		0,029						
30001	0,087							0,087	
30003	0,069	0,069							
30005	0,069							0,069	
30006	0,102			0,102					
40001		[0,3371]							
40003-1	0,068	0,068							
40003-2	0,079							0,079	
40004	0,091							0,091	
40013	0,057					0,057			
40014	0,071							0,071	
40015	0,228				0,228				
40016	0,250				0,250				
40017	0,022					0,022			
40018	0,076		0,076						
40020	0,095								0,095
40021	0,090		0,090						
40023	0,140						0,140		
40024	0,063	0,063							
40025					[0,000]				

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-12


Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	0,070		0,070						
40029	0,240				0,240				
40031	0,077								0,077
40036	0,069		0,069						
40037	0,080		0,080						
40041	0,220				0,220				
40043	0,099			0,099					
40047	0,057		0,057						
40049	0,058		0,058						
50001	0,058		0,058						
50002	0,047		0,047						
60005	0,227				0,227				
60006	0,046							0,046	
70001	0,077		0,077						
70002	0,070		0,070						
70003	0,070		0,070						

Statistical Results

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	0,087	0,069	0,068	0,101	0,233	0,040	0,088	0,070	0,082
SD	0,051	0,004	0,021	0,002	0,012	0,025	0,073	0,011	0,012
Mean - 2SD	0,000	0,061	0,027	0,096	0,209	0,000	0,000	0,048	0,058
Mean + 2SD	0,188	0,077	0,110	0,105	0,257	0,089	0,235	0,093	0,107
Amount	55	5	18	2	5	2	2	16	6

*The graphic is for information purposes only and not validated. Please read your results from the table.



Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-13

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	0,611	0,611							
3014	0,746							0,746	
3019	0,685								0,685
3025	0,670							0,670	
3027	0,757							0,757	
3028	0,740								0,740
3030	0,659							0,659	
3031	0,757								0,757
3033	0,670		0,670						
3035	0,590		0,590						
3036	0,467						0,467		
3037	0,533							0,533	
3038	0,761							0,761	
3039	0,656							0,656	
3040	0,591		0,591						
3041	0,736								0,736
3047	0,645							0,645	
3048	0,696		0,696						
3049	0,655							0,655	
13004	0,680	0,680							
15033	0,690							0,690	
20002	0,306		0,306						
30001	0,833							0,833	
30003	0,650	0,650							
30005	0,750							0,750	
30006	0,722			0,722					
40001		[2,1669]							
40003-1	0,719	0,719							
40003-2	1,003							1,003	
40004	0,599							0,599	
40013	1,200					1,200			
40014	0,687							0,687	
40015	1,680				1,680				
40016	1,500				1,500				
40017	1,140					1,140			
40018	0,482		0,482						
40020	0,715								0,715
40021	0,589		0,589						
40022									
40023	1,200						1,200		
40024	0,640	0,640							
40025					[0,001]				

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-13

Your result: The results from all participants can be found in the outstanding table.

Method	LUM		ELISA				MS	Others	
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	0,630		0,630						
40029	1,490				1,490				
40031	0,720								0,720
40036	0,663		0,663						
40037	0,580		0,580						
40041	1,310				1,310				
40043	0,829			0,829					
40047	0,533		0,533						
40049	0,558		0,558						
50001	0,675		0,675						
50002	0,634		0,634						
60005	2,111				2,111				
60006	0,471							0,471	
70001	0,568		0,568						
70002	0,520		0,520						
70003	0,660		0,660						

Statistical Results

Method	LUM		ELISA				MS	Others	
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	0,770	0,660	0,582	0,776	1,618	1,170	0,834	0,695	0,725
SD	0,325	0,041	0,092	0,076	0,305	0,042	0,518	0,121	0,025
Mean - 2SD	0,121	0,578	0,398	0,624	1,008	1,085	0,000	0,452	0,676
Mean + 2SD	1,419	0,742	0,766	0,927	2,228	1,255	1,870	0,938	0,775
Amount	55	5	18	2	5	2	2	16	6

*The graphic is for information purposes only and not validated. Please read your results from the table.

