

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-21

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	1,230	1,230							
3014	1,286							1,286	
3019	1,263							1,263	
3023	1,178							1,178	
3025	1,290							1,290	
3027	1,351							1,351	
3030	1,308							1,308	
3031									[0,192]
3032	1,159							1,159	
3033	1,319							1,319	
3035	1,130		1,130						
3036	1,380						1,380		
3037	1,453							1,453	
3038	1,377							1,377	
3039	1,408							1,408	
3040	1,217		1,217						
3041	1,473								1,473
3048	1,209		1,209						
3049	1,280							1,280	
3053	1,465		1,465						
3055	1,420								1,420
13004	1,390	1,390							
15033	1,400							1,400	
20002	0,982		0,982						
22236	1,534			1,534					
30001	1,582							1,582	
30005	1,493							1,493	
30006	1,528			1,528					
40001		[2,784]							
40002	1,087		1,087						
40003-1	1,568	1,568							
40003-2	1,740							1,740	
40004	1,134							1,134	
40013	2,490					2,490			
40014	1,316							1,316	
40015	5,140				5,140				
40017	2,250					2,250			
40020	1,580								1,580
40021	1,159		1,159						
40023	2,410						2,410		
40024	1,230	1,230							

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-21

Your result: The results from all participants can be found in the outstanding table.


Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	1,280		1,280						
40029	2,640				2,640				
40031	1,390								1,390
40036	1,048		1,048						
40037	1,450		1,450						
40038	3,240				3,240				
40041	2,260				2,260				
40043	1,513			1,513					
40047	1,208		1,208						
40048	1,370		1,370						
40049	1,172		1,172						
40051	1,284							1,284	
50001	1,469		1,469						
50002	1,583		1,583						
60006	0,928							0,928	
70001			[0,104]						
70002	1,070		1,070						
70003	1,270		1,270						

Cortisol Sample Number 21-21

Statistical Results

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	1,525	1,355	1,245	1,525	3,320	2,370	1,895	1,327	1,466
SD	0,652	0,161	0,171	0,011	1,279	0,170	0,728	0,171	0,084
Mean - 2SD	0,220	1,032	0,904	1,503	0,763	2,031	0,438	0,986	1,299
Mean + 2SD	2,830	1,677	1,586	1,547	5,877	2,709	3,352	1,669	1,633
Amount	56	4	17	3	4	2	2	20	4

*The graphic is for information purposes only and not validated. Please read your results from the table.

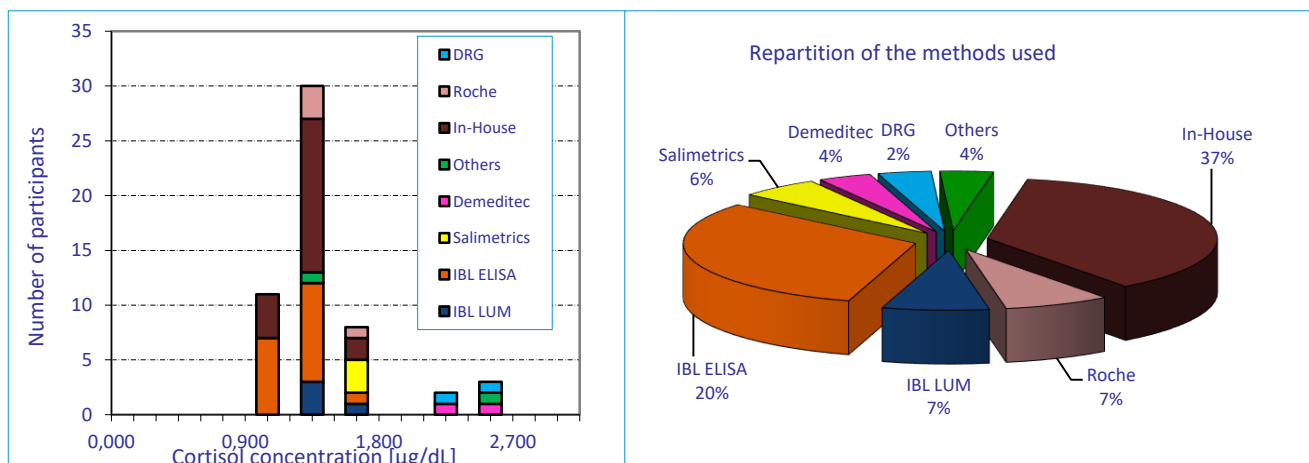

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-22

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	0,077	0,077							
3014	0,087							0,087	
3019	0,060							0,060	
3023	0,783							0,783	
3025	0,059							0,059	
3027	0,061							0,061	
3030	0,058							0,058	
3031	0,120								0,120
3032	0,058							0,058	
3033	0,055							0,055	
3035	0,050		0,050						
3036	0,105						0,105		
3037	0,065							0,065	
3038	0,069							0,069	
3039	0,062							0,062	
3040	0,047		0,047						
3041	0,085								0,085
3048	0,047		0,047						
3049	0,064							0,064	
3053	0,066		0,066						
3055	0,074								0,074
13004	0,050	0,050							
15033	0,070							0,070	
20002	0,026		0,026						
22236	0,093			0,093					
30001	0,074							0,074	
30005	0,069							0,069	
30006	0,090			0,090					
40001		[0,227]							
40002	0,065		0,065						
40003-1	0,064	0,064							
40003-2	0,084							0,084	
40004	0,080							0,080	
40013	0,075								
40014	0,072							0,072	
40015	0,232				0,232				
40017	0,260								
40020	0,126								0,126
40021	0,055		0,055						
40023	0,100						0,100		
40024	0,061	0,061							

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-22

Your result: The results from all participants can be found in the outstanding table.


Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	0,050		0,050						
40029	0,210				0,210				
40031	0,080								0,080
40036	0,057		0,057						
40037	0,090		0,090						
40038	0,230				0,230				
40041	0,170				0,170				
40043	0,084			0,084					
40047	0,060		0,060						
40048	0,085		0,085						
40049	0,046		0,046						
50001	0,058		0,058						
50002	0,062		0,062						
60006	0,040							0,040	
70001	0,083		0,083						
70002	0,050		0,050						
70003	0,060		0,060						

Cortisol Sample Number 21-22

Statistical Results

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	0,095	0,063	0,059	0,089	0,211	0,168	0,103	0,101	0,097
SD	0,104	0,011	0,016	0,005	0,029	0,131	0,004	0,161	0,024
Mean - 2SD	0,000	0,041	0,028	0,080	0,153	0,000	0,095	0,000	0,049
Mean + 2SD	0,304	0,085	0,090	0,098	0,268	0,429	0,110	0,423	0,145
Amount	57	4	18	3	4	2	2	20	5

*The graphic is for information purposes only and not validated. Please read your results from the table.



Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-23

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
3013	0,635	0,635							
3014	0,630							0,630	
3019	0,602							0,602	
3023	0,533							0,533	
3025	0,593							0,593	
3027	0,645							0,645	
3030	0,667							0,667	
3031	0,112								0,112
3032	0,580							0,580	
3033	0,583							0,583	
3035	0,470		0,470						
3036	0,652						0,652		
3037	0,674							0,674	
3038	0,652							0,652	
3039	0,520							0,520	
3040	0,645		0,645						
3041	0,745								0,745
3048	0,628		0,628						
3049	0,607							0,607	
3053	0,494		0,494						
3055	0,724								0,724
13004	0,620	0,620							
15033	0,700							0,700	
20002			[0,261]						
22236	0,775			0,775					
30001	0,764							0,764	
30005	0,736							0,736	
30006	0,755			0,755					
40001		[1,593]							
40002	0,504		0,504						
40003-1	0,723	0,723							
40003-2	0,848							0,848	
40004	0,586							0,586	
40013	1,180					1,180			
40014	0,593							0,593	
40015	1,480				1,480				
40017	1,140				1,140				
40020	0,860								0,860
40021	0,497		0,497						
40023	1,120						1,120		
40024	0,559	0,559							

Quality Assessment Scheme for Salivary Steroids

Cortisol Sample Number 21-23

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Lab. Code	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL	µg/dL
40027	0,530		0,530						
40029	1,410				1,410				
40031	0,730								0,730
40036	0,495		0,495						
40037	0,510		0,510						
40038	1,510				1,510				
40041	1,300				1,300				
40043	0,697			0,697					
40047	0,512		0,512						
40048	0,563		0,563						
40049	0,543		0,543						
40051	0,617							0,617	
50001	0,639		0,639						
50002	0,688		0,688						
60006	0,397							0,397	
70001	0,595		0,595						
70002	0,470		0,470						
70003	0,610		0,610						

Statistical Results

Method		LUM	ELISA					MS	Others
Supplier	all	IBL	IBL	Salimetrics	Demeditec	DRG	Others	In-House	Roche
Mean	0,696	0,634	0,553	0,742	1,425	1,160	0,886	0,626	0,634
SD	0,263	0,068	0,069	0,041	0,093	0,028	0,331	0,095	0,297
Mean - 2SD	0,170	0,499	0,415	0,661	1,238	1,103	0,224	0,436	0,040
Mean + 2SD	1,221	0,770	0,690	0,823	1,612	1,217	1,548	0,817	1,229
Amount	57	4	17	3	4	2	2	20	5

*The graphic is for information purposes only and not validated. Please read your results from the table.

